



RESOLVED

Safer Practice Notice

Status

Resolved

Potential for Glass-related Particles in FLOLAN® (epoprostenol sodium) Sterile Diluent and the Essential Use of a Filter with the Administration of the Reconstituted Product

The SPN originally issued on 29 Apr 2013 is now considered resolved because:


- The equipment is no longer in use
- The identified hazard no longer exists/ has been significantly reduced
- New policy is now in place
- Other

Zone Application

- Provincial
- North
- Edmonton
- Central
- Calgary
- South

Date Resolved:

06 Jan 2016

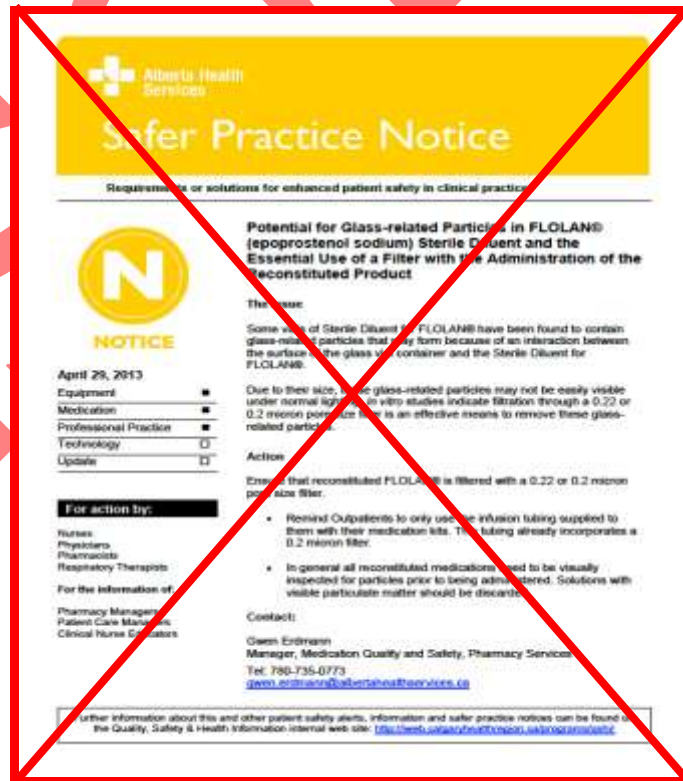

Action

- Please remove the original SPN from bulletin boards

This material is intended for use only by Alberta Health Services staff/Medical and Midwifery staffs. External readers should review the information in the context of their own environment to determine applicability. Alberta Health Services expressly disclaims all liability for the use of these materials, and for any claims, actions, demands or suits arising from such use. Further information about this and other Patient Safety Alerts and Safer Practice Notices can be found at:

<http://www.albertahealthservices.ca/patientsafety>